



Use and Care: Hand wash in cold water using mild soap. Rinse thoroughly, and air dry. If not rinsed thoroughly, soap residue may cause skin irritation and material breakdown.

Warning: This product is to be used under the supervision of a medical professional. This device is not intended for unsupervised public use. If you experience any pain, swelling, sensation changes, or any unusual reactions while using this product, consult your medical professional immediately.

Warranty: Top Shelf Orthopedics guarantees this product to be free of defects in material and construction, for a period of six months from the date of purchase on the associated soft goods and straps.

Caution: Federal Law (U.S.A.) restricts this device to sale by or on the order of a licensed health care professional. For single patient use only.

The Remedy 2.0 ER

Instructions for Use

Please read these instructions completely and carefully before applying this product. Correct application is important for proper function of this product.



The Remedy 2.0 ER

Instructions for Use





Please read these instructions completely and carefully before applying this product. Correct application is important for proper function of this product.

Indications: Immobilization and support of the shoulder/post-operative recovery

Application Instructions:

Sling & Pillow

- A. Wrap and secure waist belt with sling around the patient's waist. Open wrist and forearm strap clips and elbow closure on the sling (Image A). Trim excess strap to desired length (Image A-1).
- B. Place forearm into sling so that the hand is supported by the sling. Fasten wrist strap clip and then the forearm strap clip. The wrist and forearm should be held snugly against the pillow. Hook/loop straps may be adjusted as appropriate. (Image B-1) Secure the posterior elbow strap to the waist strap to hold the elbow against the pillow.
- C. Secure shoulder strap from the front of the abduction pillow over the affected shoulder and attach strap to the waist belt under the affected shoulder (Image C). Adjust strap as necessary for proper fit.
- D. Excess strap material may be trimmed by removing the y-tab, trim the strap length then reapply the y-tab (No image).
- E. Properly applied Remedy 2.0 ER (Image E).

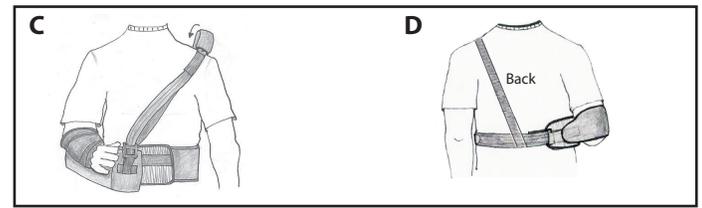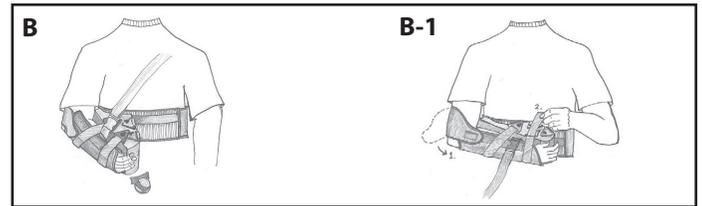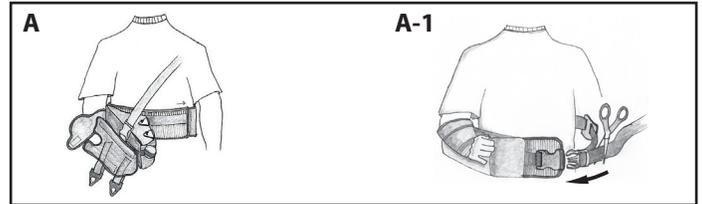

Conversion to a Shoulder Immobilizer

- F. Detach sling and sling straps from pillow. Detach pillow from sling and remove strap clips from sling straps (Image G).
- G. Attach sling to waist just below the plastic D-rings (Same Image).
- H. Wrap and secure waist belt with sling around the patient. Place forearm into sling so that the hand is supported by the sling. Feed wrist strap through D-ring and secure. Feed wrist strap through D-ring and secure. Feed forearm strap through D ring and secure (Same Image).
- I. Secure the posterior elbow strap to the waist strap to hold the elbow against the body (Same Image).
- J. Properly applied Remedy 2.0 ER without pillow (Image J).

